


MASS SPECTROMETRY REPORT

605846

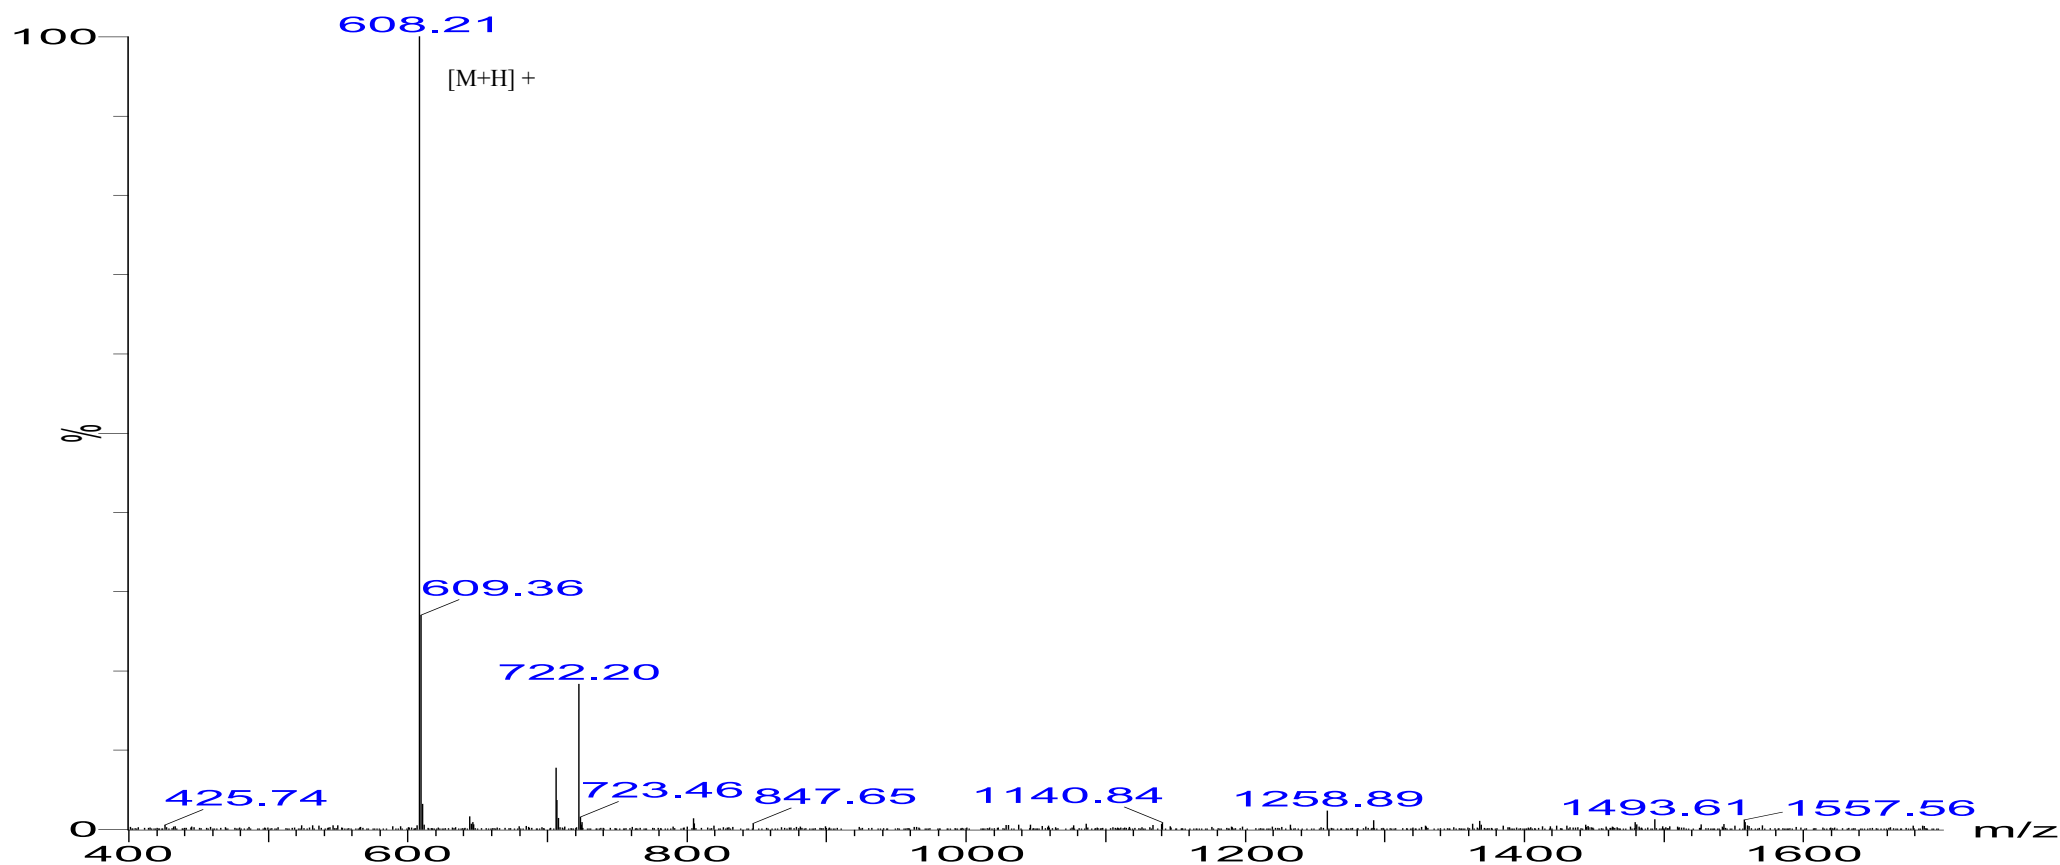

Sample Description

Analyzed date: 2025-05-26
 Analyst: SHAO
 Sample: 605846
 M.W.: 607.7
 Lot. No.:

Instrument

Probe: ESI
 Desolvation Gas Flow: 250L/Hr
 Cone: 35.0V
 Desolvation Temp.: 200 °C
 Source Temp.: 120 °C

Waters ZQ 2000

Capillary: 3.0kV
 Extractor: 3.0V
 RF Lens: 0.1V
 T. Flow: 0.5ml/min
 B. Conc.: 50%H₂O/50%ACN