



File D:\DATA\SHYY\MONITOR\MJ-796-T-13347-LCMSA044.D

Injection Date : 26 Dec 25 11:40 am +0800 Tgt Mass(EZX) : 487.00
 Sample Name : MJ-796-T Location : P1-F-05
 Acq. Operator : SHYY-MONITOR Inj : 1
 Spec. Reported : MS Integration Inj Volume : 2 ul
 Acq. Method : D:\METHODS\1-POS-5MIN.M
 Analysis Method : D:\METHODS\1-POS-5MIN.M
 Sample Info : Easy-Access Method: '1-POS-5MIN' 487.00
 Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)
 Gradient: 5%-95% B in 2.5min
 Flow Rate: 1.8 ml/min
 Column: Poroshell 120 C18 4.6*50mm, 4um
 Oven Temperature: 45 C
 UV214, MASS110-1500


*DAD1 A, Sig=214,4 Ref=off

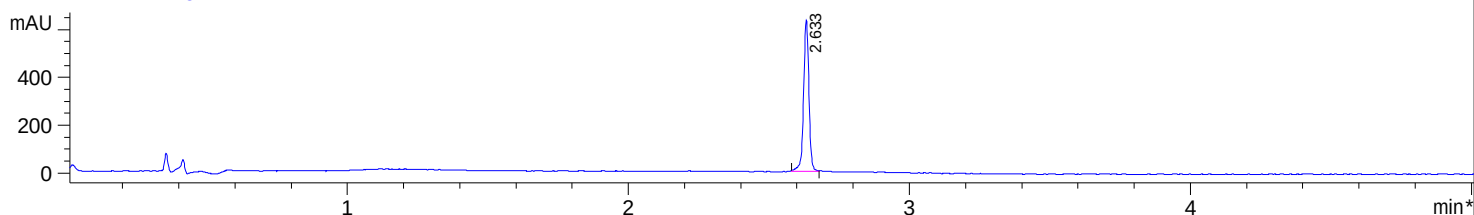


*DAD1 B, Sig=254,4 Ref=off

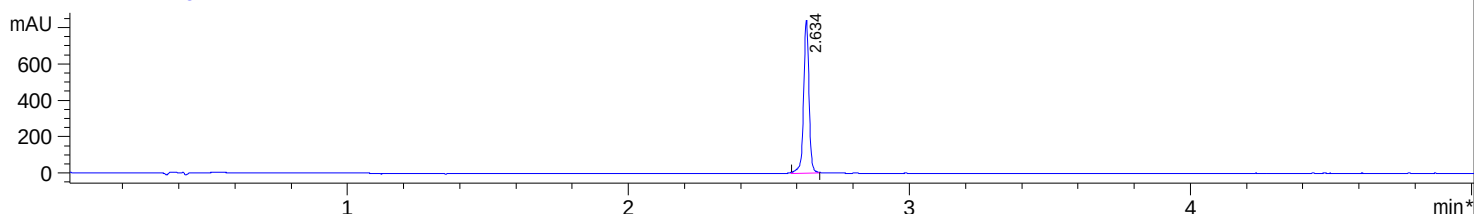

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

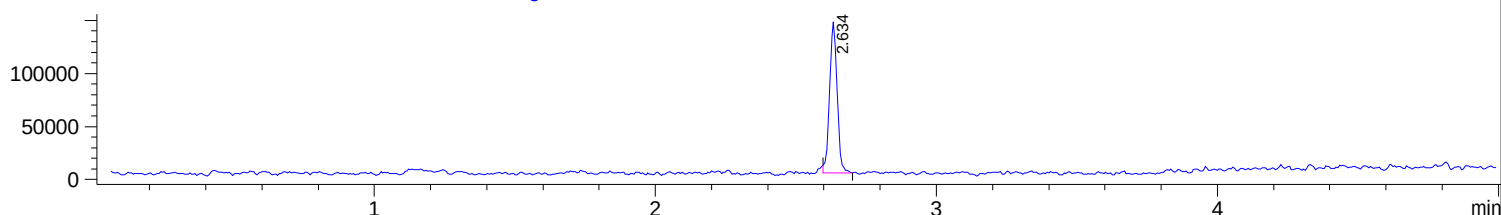

Ion 488, MSD1 488, Target Mass 487 +H Positive, EIC=487.7:488.7

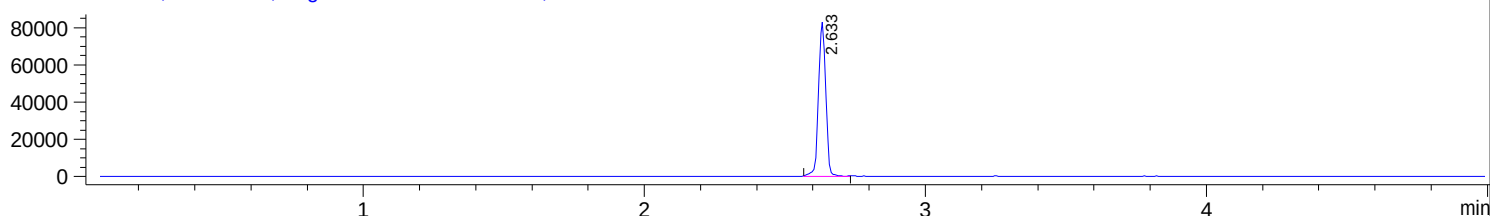

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
2.63	0.02	834.93	635.81	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
2.63	0.02	1113.25	844.37	100.00

Ret. Time: 2.63

<<<< POSITIVE SPECTRA >>>>

